


Figure 2 Bland Altman scatter

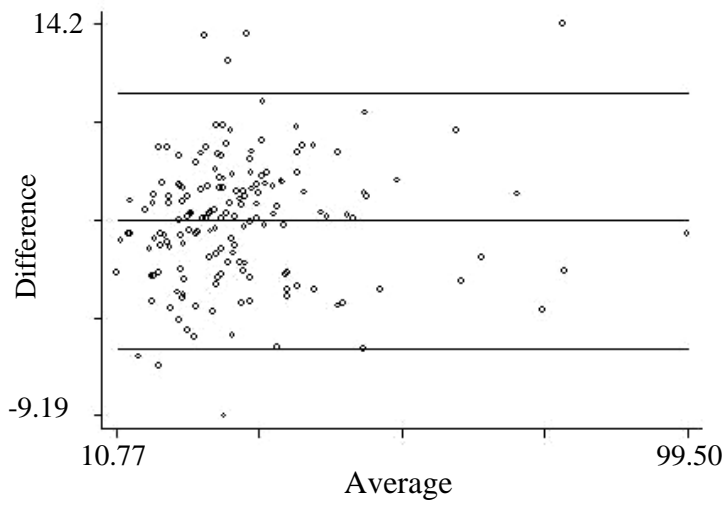

The differences between the two methods: FPIA-HPLC for Hcy measurement ($\mu\text{mol/L}$) are plotted against the averages of the two determinations. Mean of the difference ± 1.96 sem are represented by lines.